

PosiTector® *SST* Abrasives Test Kit

Addendum to Instruction Manual v.1



The Abrasives Test Kit for the **PosiTector SST** was designed to determine the concentration of soluble salts in blast cleaning abrasives, in accordance with ASTM D4940 and ISO 11127-6.

DeFelsko[®]
The Measure of Quality

Steps to Perform a Test in accordance with ASTM D4940

Test Preparation


- a) Verify the **PosiTector SST** test cell using the Certified Conductivity Standard (refer to the Quick Guide).
- b) Thoroughly rinse beakers, funnels, and stirring rod with deionized (DI) water until the rinse water has a conductivity of 5.0 $\mu\text{s}/\text{cm}$ (5.0 $\mu\text{mho}/\text{cm}$) or less.

1 - Prepare the Abrasive Solution

- a) Add 300 ml of deionized water to the 600 ml glass beaker.
- b) Using the plastic beaker, measure 300 ml of abrasive. Add to the 600 ml glass beaker.
- c) Stir the abrasive-water solution for 1 minute, let stand 8 minutes, then stir for another minute.

2 - Filter the Abrasive Solution

- a) Prepare the filter paper by folding in half, and then in half again. Place your finger between the third and fourth layers to open into a funnel shape.

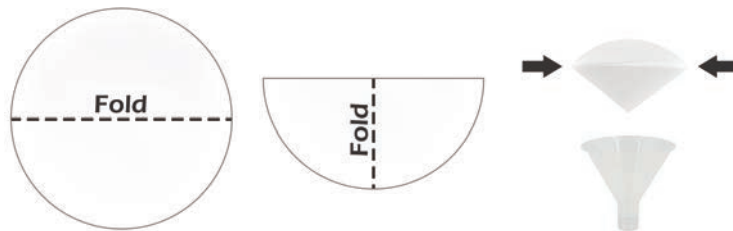

- b) Insert the filter into the plastic funnel and filter 10 ml of liquid into a separate container and discard.
- c) Using the wetted filter and funnel, continue filtering liquid into the small glass beaker to the 80 ml line.

3 - Prepare the Test Cell

Rinse the **PosiTector SST** test cell with deionized (DI) water until the rinse water has a conductivity reading of 5.0 $\mu\text{s/cm}$ (5.0 $\mu\text{mho/cm}$) or less.

Ensure the **PosiTector SST** has been taken out of **Bresle Mode** prior to testing.

4 - Test the Filtered Solution

- a) Rinse the **PosiTector SST** probe cell by submerging it into the filtered liquid 2 to 3 times.
- b) Lower the **PosiTector SST** probe cell into the filtered liquid and record the results in accordance with ASTM D4940. A calculation is not required as the test cell constant (K_{25}) is equal to 1.

An update may be needed for the **PosiTector SST** to display measurements above 500 $\mu\text{s/cm}$.

Limited Warranty, Sole Remedy and Limited Liability

DeFelsko's sole warranty, remedy, and liability are the express limited warranty, remedy, and limited liability that are set forth on its website:

This manual is copyrighted with all rights reserved and may not be reproduced or transmitted, in whole or part, by any means, without written permission from DeFelsko Corporation.

DeFelsko, PosiTector and PosiSoft are trademarks of DeFelsko Corporation registered in the U.S. and in other countries. Other brand or product names are trademarks or registered trademarks of their respective holders.

Every effort has been made to ensure that the information in this manual is accurate. DeFelsko is not responsible for printing or clerical errors.

DeFelsko[®]
Inspection Instruments

© DeFelsko Corporation USA 2018 All Rights Reserved